

Article

Portable Laser Photoacoustic Methane Sensor Based on FPGA

Jianwei Wang ^{1,*}, Huili Wang ² and Xianyong Liu ¹

¹ School of Information Engineering, Southwest University of Science and Technology, Mianyang 621010, China; wangjw@swust.edu.cn

² Joint laboratory for extreme conditions matter properties, Southwest University of Science and Technology and research center of laser fusion CAEP, Mianyang 621010, China; wanghl760@163.com

* Correspondence: wangjw@swust.edu.cn; Tel.: +86-816-608-8976

Abstract: A portable laser photoacoustic sensor based on a Field-Programmable Gate Array (FPGA) is reported for methane detection. A tunable DFB diode laser in the 1654 nm wavelength range is used as an excitation source. The photoacoustic signal processing was implemented by a FPGA device. A small resonant photoacoustic cell is designed. The minimum detection limit (1σ) of 10 ppm for methane (CH_4) is demonstrated.

Keywords: FPGA; photoacoustic spectroscopy; diode laser; methane

1. Introduction

Methane (CH_4) detection plays an important role in various applications, such as natural gas exploration, coal mining, medical diagnostics and environment monitoring [1-5]. There exist numerous CH_4 sensing devices based on different detection principles like catalytic combustion, gas chromatography (GC), electrochemical sensors, semiconductor, infrared spectroscopy, etc [6-8]. Compared with the above sensors, the main advantages of laser photoacoustic (PA) gas sensors are the high sensitivity, large dynamic range, without the need for sample preparation and in situ measurements.

PA detection of trace gases is one of the most sensitive techniques of infrared absorption spectroscopy [9-12]. The success of PA gas detection crucially depends on the availability and performance of excitation light sources in combined with appropriate detection schemes. There are several of factors effecting on PA gas detection technology. The two main factors are light sources and weak signal detection technique. Tunable near-infrared diode lasers and tunable mid-infrared quantum cascade lasers (QCLs) are generally employed as excitation light sources today [13-15]. The tunable distributed feedback (DFB) diode laser is the appropriate laser source for portable gas sensor due to its compact shape and stability characteristics [16-20]. The weak signal detection technique for the PA gas detection is another key factor. The use of commercial lock-in amplifier makes the PA gas detection system obtain high sensitivity. These gas detection systems based on commercial lock-in amplifier (Stanford Research Systems, SR830) are hardly integrated and miniaturized for their relatively large volume. With rapid development of the field programmable gate arrays (FPGA) technology, the FPGA has extended the application of digital signal processing to a larger field of instrumentation in recent years [21-24]. The FPGA technology makes the sensors portable, reconfigurable and reprogrammable with the advantages of good low-cost, high integration and high-performance signal processing [25-28]. The digital lock-in amplifier based FPGA may provide new opportunity for portable PA gas detection device.

In this paper, a portable PA methane sensor based on FPGA in combination with a tunable distributed feedback (DFB) diode laser is developed. The performance of the sensor is demonstrated by the measurements of CH_4 . A detection limit of 10 ppm is obtained.

2. Sensor Design

A schematic of the portable PA methane sensor is shown in Figure 1. A tunable DFB, fiber-coupled diode laser (NLK1U5EAAA, Central Wavelength $1653.72 \pm 0.05 \text{ nm}$, 10 mW, FC/PC pigtailed, NEL, Japan) is used as the excitation light source. The laser beam is collimated using a fiber optical collimator (Operating Wavelength 1650nm, Primanex, China) for direct installations in the resonant PA cell. The DFB diode laser is operated in wavelength modulation mode by the laser controller. Modulation of the laser current is performed by applying a sinusoidal dither to the direct current ramp of the DFB diode laser at half of the PA cell's resonance frequency. The PA signals are detected by a Microphone (EK3033, 22mV/Pa) which is placed in the middle of the PA cell resonator. The amplified PA signals by a high input impedance preamplifier (AD8221, ANALOG DEVICES, USA) are measured using the lock-in amplifier based on FPGA with a time constant 1s. Gas concentration is displayed in digital display after the data acquisition and processing. The photograph of the portable PA sensor is shown in Figure 2 (220×200×80).

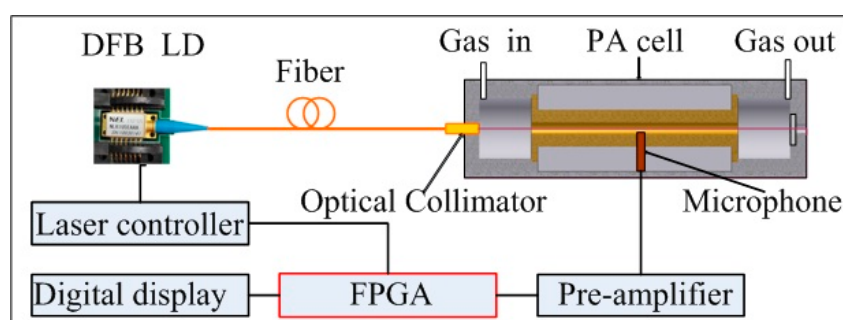


Figure 1. Schematic configuration of the PA methane sensor



Figure 2. The photograph of this PA methane sensor

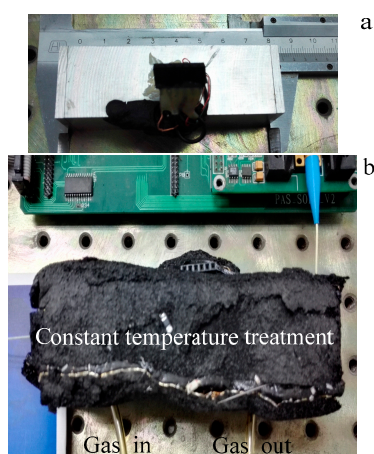


Figure 3. The PA cell and the constant temperature treatment device

In order to achieve portable gas sensor, a small resonant PA cell is designed. The shape size of this PA cell is shown in Figure 3(a). The diameter and length of the brass resonator are respectively 4 mm and 36 mm. The length of two buffer volumes is 18 mm, and their diameters are 20 mm. The length of both ends flanges is 2 mm. The end of the PA cell is sealed by a quartz window. The PA cell is highly insulated with special material to reduce the environmental temperature and humidity

interferences (see Figure 3(b)). A temperature controller accurately controls the temperature of PA cell to keep 35 degree. Under this condition the PA cell's resonance is obtained. Under this condition the PA cell's resonance is obtained (see Figure 4). The frequency, half-width and Q-factor of the resonance have been determined by extracting parameters from a Lorentzian fit. For this cell, the resonant frequency is 2450 Hz and the Q-factor is about 26 at atmospheric pressure.

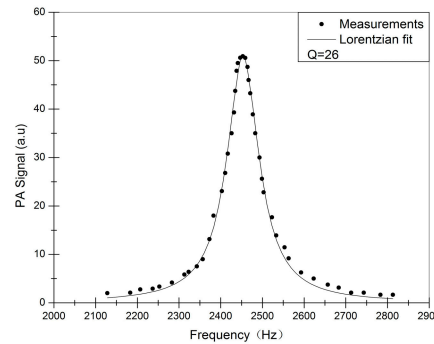


Figure 4. The resonance profiles showing the first longitude resonance frequency is 2450Hz.

The lock-in amplifier based on FPGA can be seen in Figure 5. The lock-in amplifier is implemented in a ProASIC3 series of low cost, low power FPGA (ProASIC3EL, ACTEL, USA). The FPGA is configured on a NIOS II processor with C programming language. Implementing components in FPGA allows all operations after AD sampling to be done digitally at high speed. The workflow and each functional modules of the FPGA are coordinated by this NIOS II processor [29,30]. Gas concentration is achieved to implement a computation repeatedly, composed of a series of ordered operations on a set of PA signal data. Concentrations can be directly routed to a DAC as well as displayed.

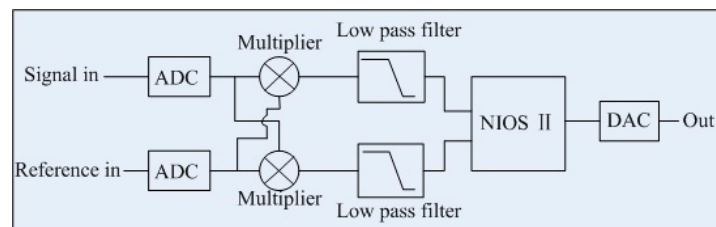


Figure 5. Schematic diagram of the FPGA based lock in amplifier.

It is assumed that the PA signal is $X1 = V_s \cos(\omega t + \theta)$, one reference signal is $R1 = V_r \cos(\omega t + \phi)$, another orthogonal reference signal is $R2 = V_r \sin(\omega t + \phi)$. When the PA signal $X1$ is separately multiplied with the reference signal $R1$ and $R2$, the results are low pass filtered yielding

$$I = kV_s V_r \cos \theta \quad (1)$$

$$Q = kV_s V_r \sin \theta \quad (2)$$

According to formula (1) and formula (2), the phase difference and the amplitude can now be calculated by this NIOS II processor

$$V_s = \frac{1}{kV_r} \sqrt{I^2 + Q^2}, \quad \theta = \arctan\left(\frac{Q}{I}\right) \quad (3)$$

where V_s is the amplitude the PA signal, θ is the phase difference of the PA signal.

The unit of sample gas preparation consists of two mass flow controllers (MFC) and two bottles of certified gas (5000 ppm CH₄ and air). Two MFCs were used to dilute certified CH₄ gas. From 100 ppm to 5000 ppm, different concentrations of CH₄ were generated by the sample gas preparation unit. For reducing excessive flow noise resulting from turbulence in the PA cell, a total flow of 100 sccm (standard cubic centimetre per minute) was used.

3. Results and Discussion

Carbon dioxide (CO₂) and water vapour (H₂O) are the most ubiquitous gas in the environment, which have infrared absorption characterization. Therefore the spectral overlap interference of none-measured gas to CH₄ detection needs to be solved. An absorption line at 1653.7 nm is selected for CH₄ detection by analyzing spectral range of center wavelength and light source characters (see Figure 6). The absorption spectrum of H₂O, CH₄ and CO₂ between 1620-1680 nm obtained from the HITRAN database [31]. Figure 6 shows there is no spectral overlap interferences at 1653.7 nm.

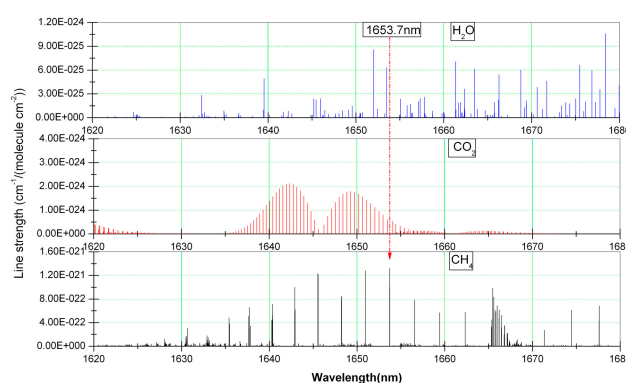


Figure 6. Absorption spectrum of the gases (H₂O, CO₂ and CH₄) obtained from the HITRAN database.

The DFB diode laser was operated under control of the operating system. The spectral of 1653.7 nm was obtained by varying the laser operating temperature from 10 to 40 °C. The sensor was used to measure the CH₄. The measured 1f spectra of 200 ppm CH₄ is shown in Figure 7.

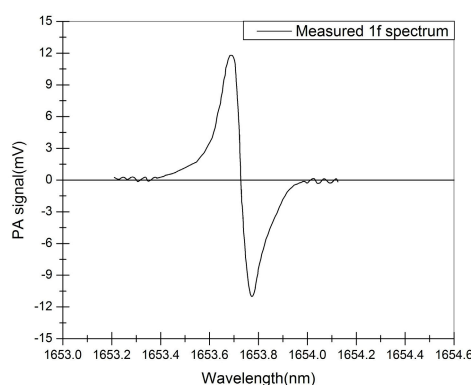


Figure 7. Measured 1f spectra of 200 ppm CH₄.

To test the sensor performance, different concentrations ranging from 100 ppm to 2000 ppm were prepared by diluting certified methane with the unit of sample gas preparation. The PA signal amplitude of different concentrations was measured as seen in Figure 8. Each dot is an average of 10 individual measurements. A linear fit was applied to obtain the linearity of the sensor. Experiments show that the PA sensor has good performance.

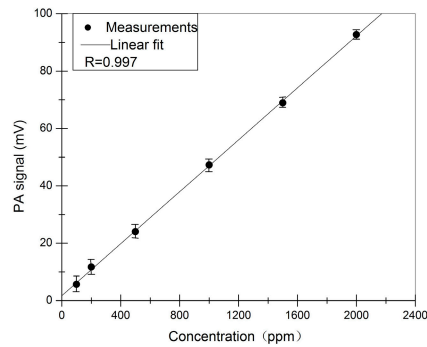


Figure 8. PA signals to different concentrations. Error bars give the range of the corresponding PA signals.

The detection limit and response time of this PA methane sensor were evaluated by detecting the PA signal with diluting calibrated mixture of 5000 ppm CH₄ in air. Both targeted and detected CH₄ concentrations were demonstrated as shown in Figure 9. The standard deviation (σ) of the PA signal is 0.52. The PA signal amplitude of 223 ppm is 11.9 mV, so a SNR of 23 was calculated, which indicated that the detection limit (SNR=1) of this PA sensor for CH₄ is about 10 ppm. The response time is about 4s. There are some differences between the targeted gas and measured CH₄ concentrations. One of the main reasons is most likely the precision of the unit of sample gas preparation during the dilution process.

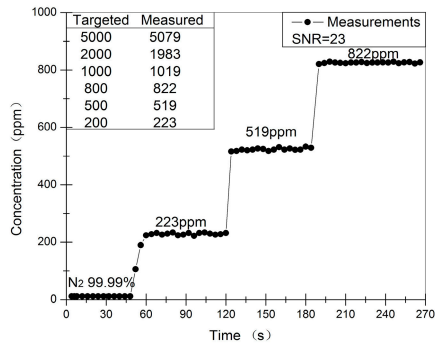


Figure 9. Measured dilution process of the 5000 ppm CH₄ reference concentration.

The PA signals of 2000 ppm CH₄ were measured for evaluating measurement stability of this PA sensor(see Figure 10). The CH₄ concentrations were displayed in digital display, which these values were recorded at intervals of 30 s. Its relative error is less than 0.5%. Measurement results show that this sensor has good stability.

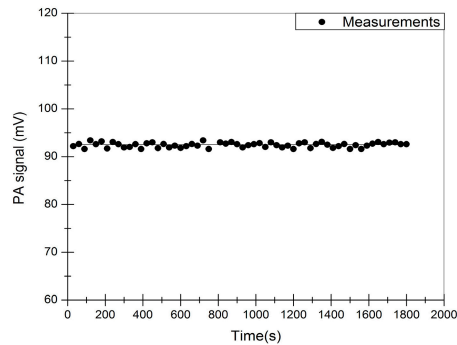


Figure 10. Continuous measurements of 2000 ppm CH₄.

4. Conclusions

A new gas sensor was developed, which used a DFB diode laser, FPGA lock-in, and resonant photoacoustic spectroscopy. The PA methane sensor is portable, compact, easy operation and intuitive display. The minimum detection limit of 10 ppm for CH₄ was demonstrated at atmospheric pressure. Further improvement is carrying out for improving the detection sensitivity by optimizing design for the FPGA lock-in. This sensor shows a possibility of supplying a new instrument for coal mine methane detection, the environmental monitoring and industrial applications in combined with appropriate detection schemes.

Acknowledgments: This work was supported by a grant from the Natural Science Foundation of Southwest University of Science and Technology (No. 12zx7126) and the Natural Science Fund of Education Department of Sichuan province (No.16zd1124).

Author Contributions: Jian-wei Wang, Hui-li Wang and Xian-yong Liu conceived and designed the experiments; Hui-li Wang performed the experiments; Jian-wei Wang and Hui-li Wang analyzed the data; Jian-wei Wang contributed the idea; Jian-wei Wang and Hui-li Wang contributed the experimental results and all of figures in measurements Jian-wei Wang wrote the paper.

Conflicts of Interest: The authors declare no conflict of interest.

References

- Li, J.; Lu, X.T.; Yang, Z.H. Remote system of natural gas leakage based on multi-wavelength characteristics spectrum analysis. *Spectrosc Spect Anal* **2014**, *34*, 1249-1252.
- Jahjah, M.; Ren, W.; Stefanski, P.; Lewicki, R.; Zhang, J.W.; Jiang, W.Z.; Tarka, J.; Tittel, F.K. A compact qcl based methane and nitrous oxide sensor for environmental and medical applications. *Analyst* **2014**, *139*, 2065-2069.
- Karacan, C.Ö.; Ruiz, F.A.; Cotè, M.; Phipps, S. Coal mine methane: A review of capture and utilization practices with benefits to mining safety and to greenhouse gas reduction. *Int J Coal Geol* **2011**, *86*, 121-156.
- Cheng, Y.-P.; Wang, L.; Zhang, X.-L. Environmental impact of coal mine methane emissions and responding strategies in china. *Int J Greenh Gas Con* **2011**, *5*, 157-166.
- Costello, B.P.J.D.; Ledochowski, M.; Ratcliffe, N.M. The importance of methane breath testing: A review. *J Breath Res* **2013**, *7*.
- Shemshad, J.; Aminossadati, S.M.; Kizil, M.S. A review of developments in near infrared methane detection based on tunable diode laser. *Sensor Actuat B-Chem* **2012**, *171*, 77-92.
- Wang, C.J.; Sahay, P. Breath analysis using laser spectroscopic techniques: Breath biomarkers, spectral fingerprints, and detection limits. *Sensors-Basel* **2009**, *9*, 8230-8262.
- Sigrist, M.W.; Bartlome, R.; Marinov, D.; Rey, J.M.; Vogler, D.E.; Wachter, H. Trace gas monitoring with infrared laser-based detection schemes. *Appl Phys B-Lasers O* **2008**, *90*, 289-300.
- Wang, J.; Zhang, W.; Liang, L.; Yu, Q. Tunable fiber laser based photoacoustic spectrometer for multi-gas analysis. *Sensor Actuat B-Chem* **2011**, *160*, 1268-1272.
- Jahjah, M.; Jiang, W.Z.; Sanchez, N.P.; Ren, W.; Patimisco, P.; Spagnolo, V.; Herndon, S.C.; Griffin, R.J.; Tittel, F.K. Atmospheric ch₄ and n₂o measurements near greater houston area landfills using a qcl-based qepas sensor system during discover-aq 2013. *Opt Lett* **2014**, *39*, 957-960.
- Patel, C.K.N. Laser photoacoustic spectroscopy helps fight terrorism: High sensitivity detection of chemical warfare agent and explosives. *Eur Phys J-Spec Top* **2008**, *153*, 1-18.
- Rocha, M.V.; Stel, M.S.; Silva, M.G.; Paiva, L.B.; Pinheiro, F.W.; Miklos, A.; Vargas, H. Quantum-cascade laser photoacoustic detection of methane emitted from natural gas powered engines. *Appl Phys B-Lasers O* **2012**, *106*, 701-706.
- Holthoff, E.L.; Heaps, D.A.; Pellegrino, P.M. Development of a mems-scale photoacoustic chemical sensor using a quantum cascade laser. *Ieee Sens J* **2010**, *10*, 572-577.
- Sampaolo, A.; Patimisco, P.; Giglio, M.; Vitiello, M.; Beere, H.; Ritchie, D.; Scamarcio, G.; Tittel, F.; Spagnolo, V. Improved tuning fork for terahertz quartz-enhanced photoacoustic spectroscopy. *Sensors-Basel* **2016**, *16*, 439.
- W.Sigrist, M. Trace gas monitoring by laser photoacoustic spectroscopy and related techniques (plenary). *Rev. Sci. Instrum.* **2003**, Vol. 74,, 485-490.
- Hanyecz, V.; Mohacsi, A.; Pogany, A.; Varga, A.; Bozoki, Z.; Kovacs, I.; Szabo, G. Multi-component photoacoustic gas analyzer for industrial applications. *Vib Spectrosc* **2010**, *52*, 63-68.

17. Besson, J.P.; Schilt, S.; Thevenaz, L. Sub-ppm multi-gas photoacoustic sensor. *Spectrochim Acta A* **2006**, *63*, 899-904.
18. Webber, M.E.; Pushkarsky, M.; Patel, C.K.N. Fiber-amplifier-enhanced photoacoustic spectroscopy with near-infrared tunable diode lasers. *Appl Optics* **2003**, *42*, 2119-2126.
19. Kosterev, A.A.; Bakhirkin, Y.A.; Tittel, F.K. Methane detection by means of quartz enhanced photoacoustic spectroscopy in nir. *2007 Conference on Lasers & Electro-Optics/Quantum Electronics and Laser Science Conference (Cleo/QELS 2007), Vols 1-5* **2007**, 1603-1604.
20. Ma, Y.; Yu, G.; Zhang, J.; Yu, X.; Sun, R.; Tittel, F. Quartz enhanced photoacoustic spectroscopy based trace gas sensors using different quartz tuning forks. *Sensors-Basel* **2015**, *15*, 7596.
21. Bernard-Schwarz, M.; Zwick, W.; Wenzel, L.; Klier, J.; Groschl, M. Field programmable gate array-assigned complex-valued computation and its limits. *Rev Sci Instrum* **2014**, *85*.
22. Schwettmann, A.; Sedlacek, J.; Shaffer, J.P. Field-programmable gate array based locking circuit for external cavity diode laser frequency stabilization. *Rev Sci Instrum* **2011**, *82*.
23. Takeda, K. A highly integrated fpga-based nuclear magnetic resonance spectrometer. *Rev Sci Instrum* **2007**, *78*.
24. Restelli, A.; Abbiati, R.; Geraci, A. Digital field programmable gate array-based lock-in amplifier for high-performance photon counting applications. *Rev Sci Instrum* **2005**, *76*.
25. Jinghong, L.; Kai, L.; Peng, Y. In *Design and implementation of flame combustion state detection system based on fpga*, Control and Decision Conference, 2015.
26. Botella, G.; Martín H., J.A.; Santos, M.; Meyer-Baese, U. Fpga-based multimodal embedded sensor system integrating low- and mid-level vision. *Sensors-Basel* **2011**, *11*, 8164.
27. González, D.; Botella, G.; Meyer-Baese, U.; García, C.; Sanz, C.; Prieto-Matías, M.; Tirado, F. A low cost matching motion estimation sensor based on the nios ii microprocessor. *Sensors-Basel* **2012**, *12*, 13126.
28. Rodríguezdonate, C.; Botella, G.; García, C.; Cabalopez, E.; Prietomatias, M. In *Early experiences with opencl on fpgas: Convolution case study*, IEEE International Symposium on Field-Programmable Custom Computing Machines, 2015; pp 235-235.
29. González, D.; Botella, G.; García, C.; Prieto, M.; Tirado, F. Acceleration of block-matching algorithms using a custom instruction-based paradigm on a nios ii microprocessor. *Journal on Advances in Signal Processing* **2013**, *2013*, 1-20.
30. Windh, S.; Ma, X.; Halstead, R.J.; Budhkar, P.; Luna, Z.; Hussaini, O.; Najjar, W.A. High-level language tools for reconfigurable computing. *Proceedings of the IEEE* **2015**, *103*, 390-408.
31. Rothman, L.S.; Gordon, I.E.; Barbe, A.; Benner, D.C.; Bernath, P.E.; Birk, M.; Boudon, V.; Brown, L.R.; Campargue, A.; Champion, J.P., et al. The hitran 2008 molecular spectroscopic database. *J Quant Spectrosc Ra* **2009**, *110*, 533-572.



© 2016 by the authors; licensee *Preprints*, Basel, Switzerland. This article is an open access article distributed under the terms and conditions of the Creative Commons by Attribution (CC-BY) license (<http://creativecommons.org/licenses/by/4.0/>).